



800 Hudson Way, Huntsville, AL 35806

P: 844-443-6663 | F: 256-327-0981

Testing Performed By Alimetric - CLIA #: 01D2113023

Medical Director: Dr. Richard V. Spera MD, FACP

simplytest.com |

FINAL REPORT

PREMIUM

Sample Type: Saliva

Reported: 03/20/2023 14:31

All values are reported in genomic copies x1000/mL

PATIENT INFO

DOB: 09/20/1980 (40 yrs)

Gender: Female

ID#: 951750

Location: Test Site A

SAMPLE INFO

Specimen#: 5555550005

Accession#: 777000-12345

Collected: 03/15/2023

Received: 03/20/2023 09:57

ORDERING PROVIDER

Glenn Close MD

8977 Lone Peak Parkway

Draper, UT 84020

800-555-5555


Low

Medium

High



NON-VIRAL TARGETS (In Range Results)

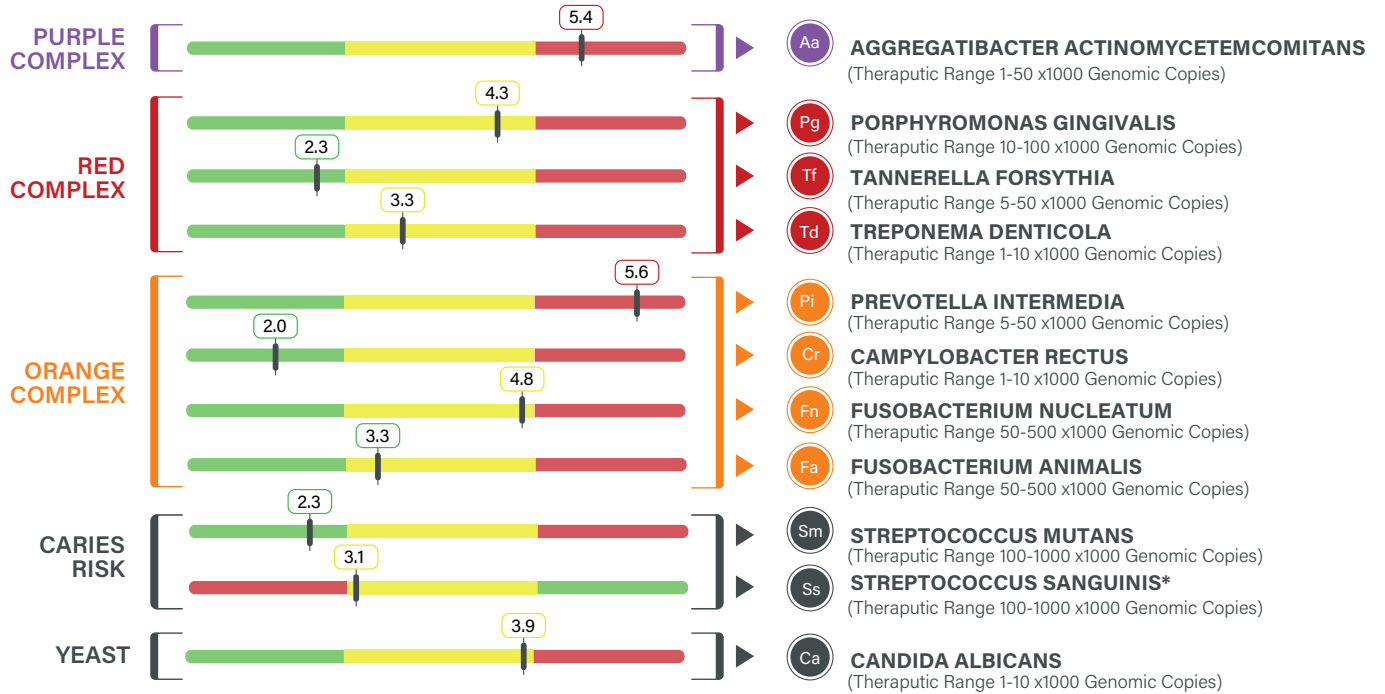

*The presence of Streptococcus Sanguinis is associated with healthy plaque biofilm.

POSITIVE	NEGATIVE	ATTENTION	VIRAL TARGETS PREMIUM ADDITIONS
	✓		HERPES SIMPLEX VIRUS 1 (HSV-1)
	✓		HERPES SIMPLEX VIRUS 2 (HSV-2)
	✓		CYTOMEGALOVIRUS
	✓		EPSTEIN BARR VIRUS



COMMENTS + ACTIONABLE CLINICAL INSIGHTS

[Lab supervisor/manager comment field]